


SALES DRAWING ONLY
NOT TO BE USED FOR MANUFACTURE

IMPORTANT

The sensor vent tube must be positioned so to prevent direct ingress of moisture.
 The Vent Filter Assembly must remain intact, if the cable is shortened for any reason the filter assembly must immediately be transfer from the off cut to the new termination of the cable.
 The transmitter cable should have 360° screen terminated in the gland of the termination enclosure.
 For gauge transmitters ensure the cable end & termination housing are located in a vented area so the breather tube can reference the transmitter cell to atmosphere.
 An extended vent tube (customer supply) must be fitted in areas where flooding or hose wash down are likely.
 6mm (1/4") od plastic tube is suitable and should run to a dry area which is at the same atmospheric pressure as with in the tank.

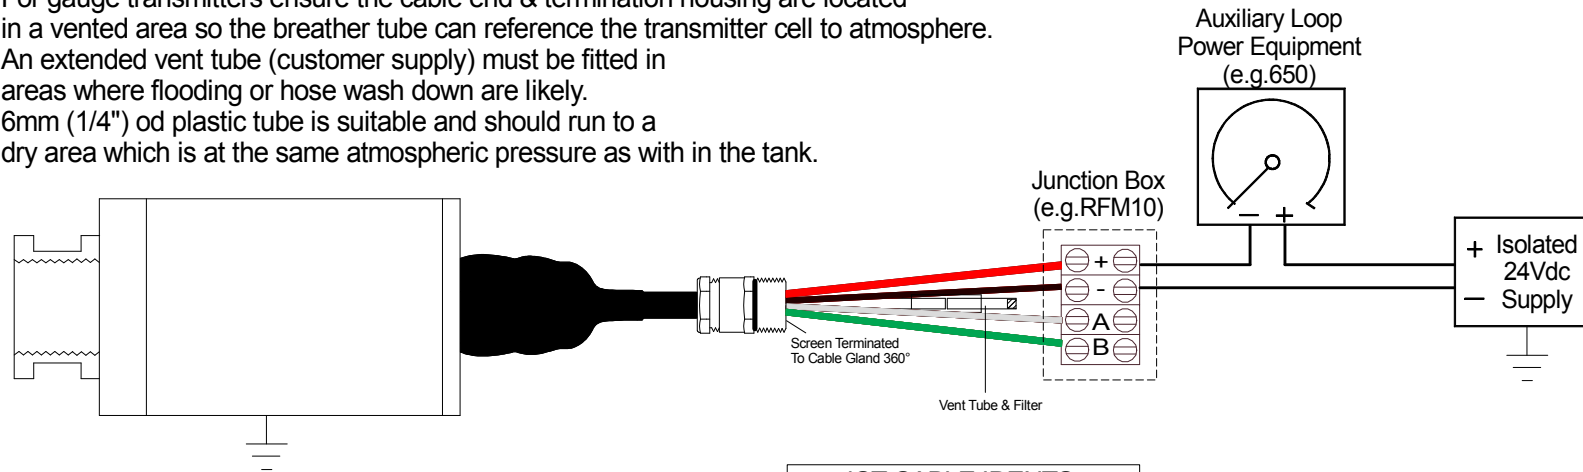

iCT CABLE IDENTS		
Red	+ Positive	Supply
Black	- Negative	4-20mA
White	A Data +	RS485 Modbus
Green	B Data -	

ISSUE	DATE	DCR	DRAWN	CHECKED
A	28-04-08		JEK	
B	02-07-14			SAL
C	19-12-14			SAL
D	14-02-17			SAL

PSm Instrumentation Ltd

Haywards Heath, West Sussex RH16 1TW
 ph: 44 (0) 1444 410040 f: 44 (0) 1444 410121
<http://www.psmmarine.com>

SCALE
NTS

UNLESS OTHERWISE STATED DIMENSIONS ARE IN
MILLIMETRES / INCHES

TITLE
ICT Analogue 4-20mA
Hookup Drawing

DRAWING NO
S-001309-ICT-GO

A4

SHT 1
OF 1