



SALES DRAWING ONLY
NOT TO BE USED FOR MANUFACTURE

MODEL	Flange	Holes	PCD	Hole Dia	A	B
A6	DN25 PN16	4	85	14	115	16

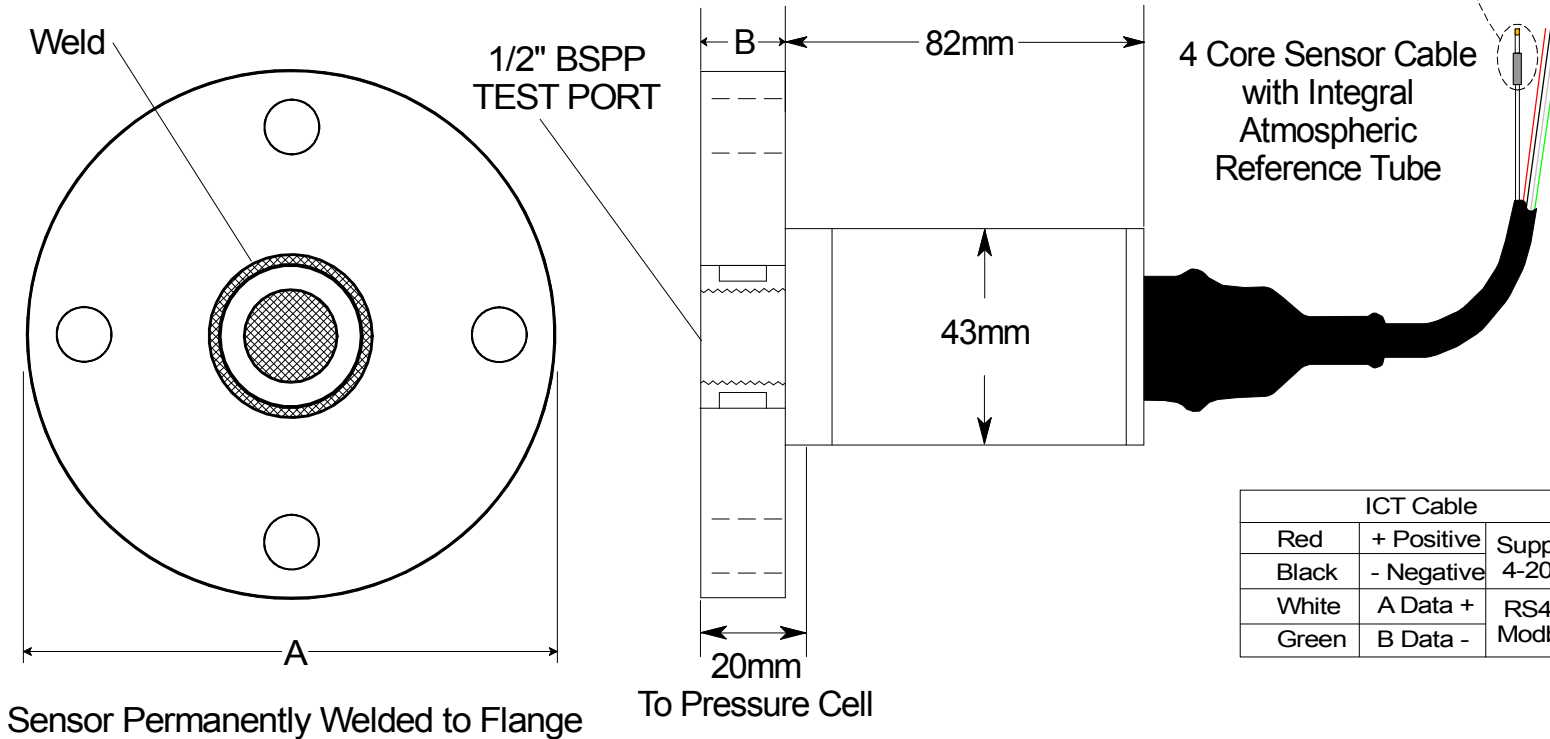

Removeable filter assembly must always be connected to the vent tube. If the cable is shortened then this assembly must be fitted to the new cable end.



ICT Cable		
Red	+ Positive	Supply & 4-20mA
Black	- Negative	
White	A Data +	RS485 Modbus
Green	B Data -	

ISSUE	DATE	DCR	CHECKED	A	B	C	D
	28/08/14		MVJ	SAL	MVJ		
						09-04-15	02-07-15
						SAL	SAL
						MVJ	MVJ

PSm Instrumentation Ltd
 Haywards Heath, West Sussex RH16 1TW
 ph: 44 (0) 1444 410040 f: 44 (0) 1444 410121
<http://www.psmmarine.com>

SCALE
NTS

UNLESS OTHERWISE STATED DIMENSIONS ARE IN
MILLIMETRES / INCHES

TITLE
ICT1000 Model A6
DN25 PN16 Flange

DRAWING NO
S-001406-ICT-DD

A4 SHT 1 OF 1